


Basic Kill+ with Advanced viaDNA Remote – White Box

Select the spooky2 software **Settings** tab

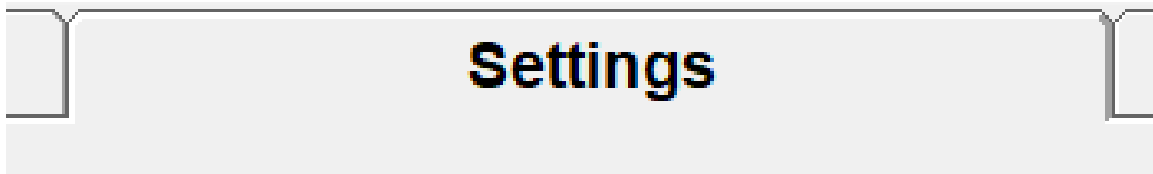

In the **Signal Settings** box type in the **Amplitude** and **Offset** numbers for **Out1** and **Out2**


Signal Settings		Out 1	Out 2	
Duty Cycle		50	50	%
Amplitude		7	7	V
Offset		100	100	%
Phase		0	0	°

In the **Output Control** box ... select **Out2 Follows Program Frequency**

Output Control	
Out 1 =	0 X
Swap Waveform Every	
<input type="radio"/>	Out 2 = (Out 1 X
<input type="radio"/>	Out 1 fixed at
<input checked="" type="radio"/>	Out 2 Follows Program Frequency
<input type="radio"/>	Out 2 Runs Every Second Frequency

Basic Kill+ with Advanced viaDNA Remote – White Box

In the **Waveform Setup** box ... select **Square Waveform** for 1 and 2

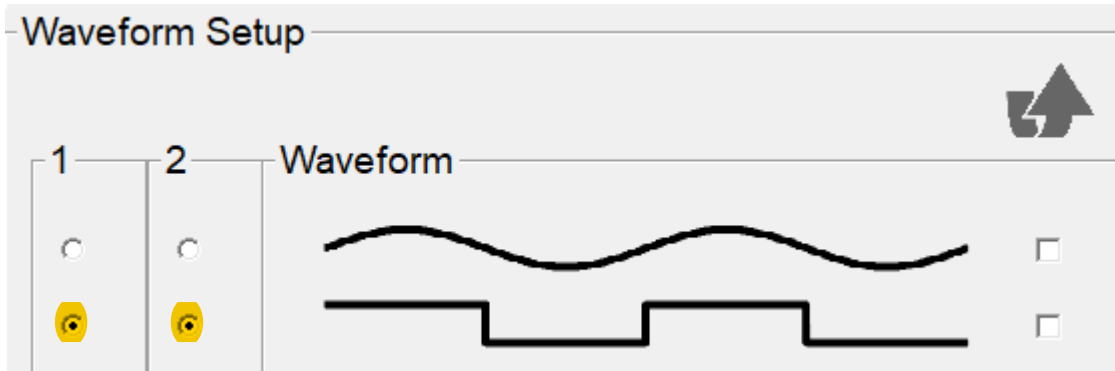

The oscilloscope box (right hand side of Settings window) should look like this

